Print on plain white paper - Part # 122919 (BOTH SIDES)

INSTALLATION INSTRUCTIONS for the *LR Assistant's Instrument Holder*

SECTION I - chair with Vac Pack

Follow the steps in Section I if your chair has the Vac Pack System already installed:

1. Remove the two button head screws from the Vac Pack cover (See Figure 1).
2. Position the instrument holder assembly as shown and Install it to the chair using the two socket head screws provided (See Figure 2).

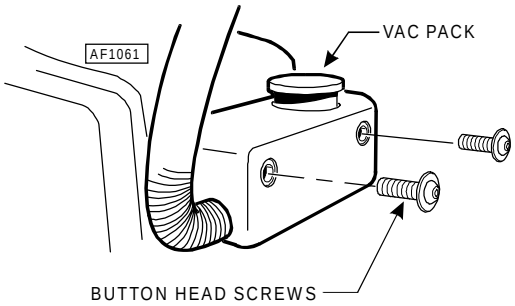

Figure 1

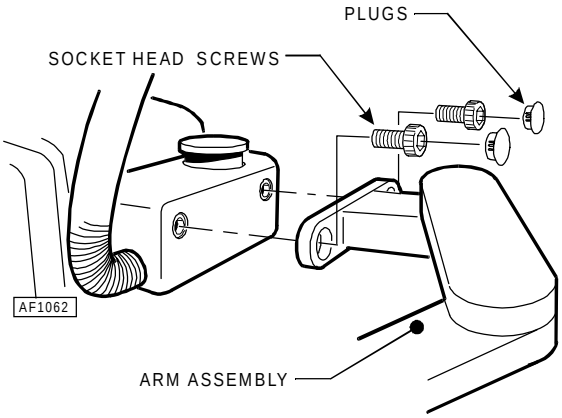

Figure 2

SECTION II - chair without Vac Pack

Follow the steps in Section II if your chair does not have the Vac Pack System:

1. Remove the three Platform covers as shown (See Figure 3). Discard the center platform cover.
2. Insert the spacers provided in the holes in the new platform cover and position the cuspidor assembly as shown. Install the assembly to the chair platform using the two socket head screws provided (See Figure 4).
3. Replace the covers.

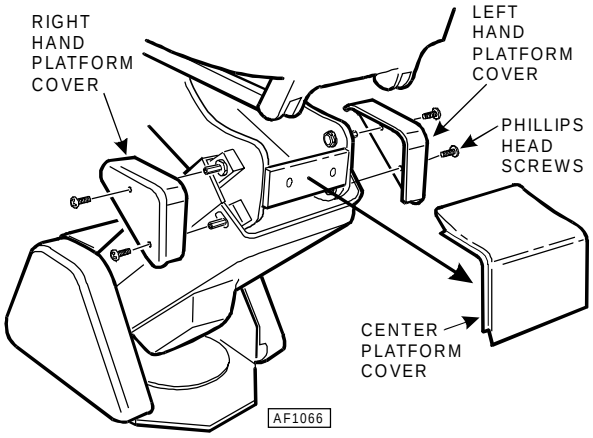

Figure 3

SECTION III - Height adjustment

The height of the instrument holder can be easily adjusted by the following procedure:

1. While supporting the instrument holder, Loosen the upper adjustment sleeve by turning it counterclockwise until the post can be moved up and down.(See Figure 5).
2. Slide the post up or down to the desired height and tighten the sleeve firmly.

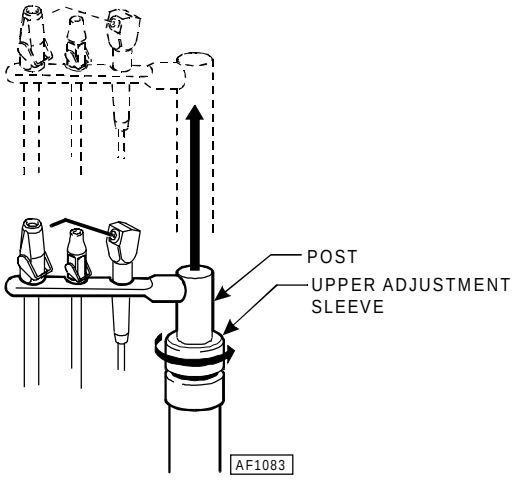

Figure 5

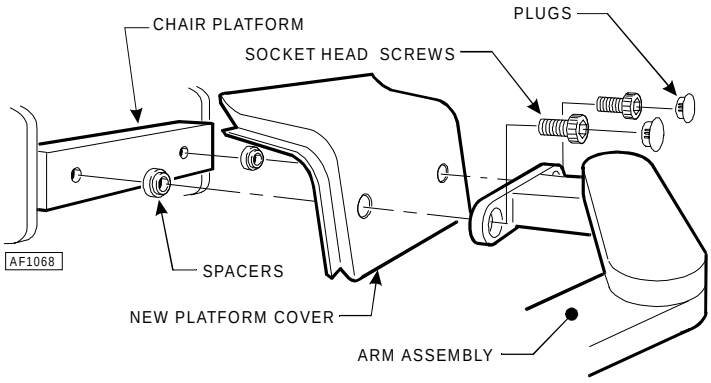

Figure 4

Knight®
by Midmark

Midmark Corporation • P O Box 286 • 60 Vista Drive
Versailles • Ohio • 45380-0286 • www.midmark.com
Phone: 937-526-3662 Fax: 937-526-5542